




STERIS drawings do not supersede the drawings from the architect of record.

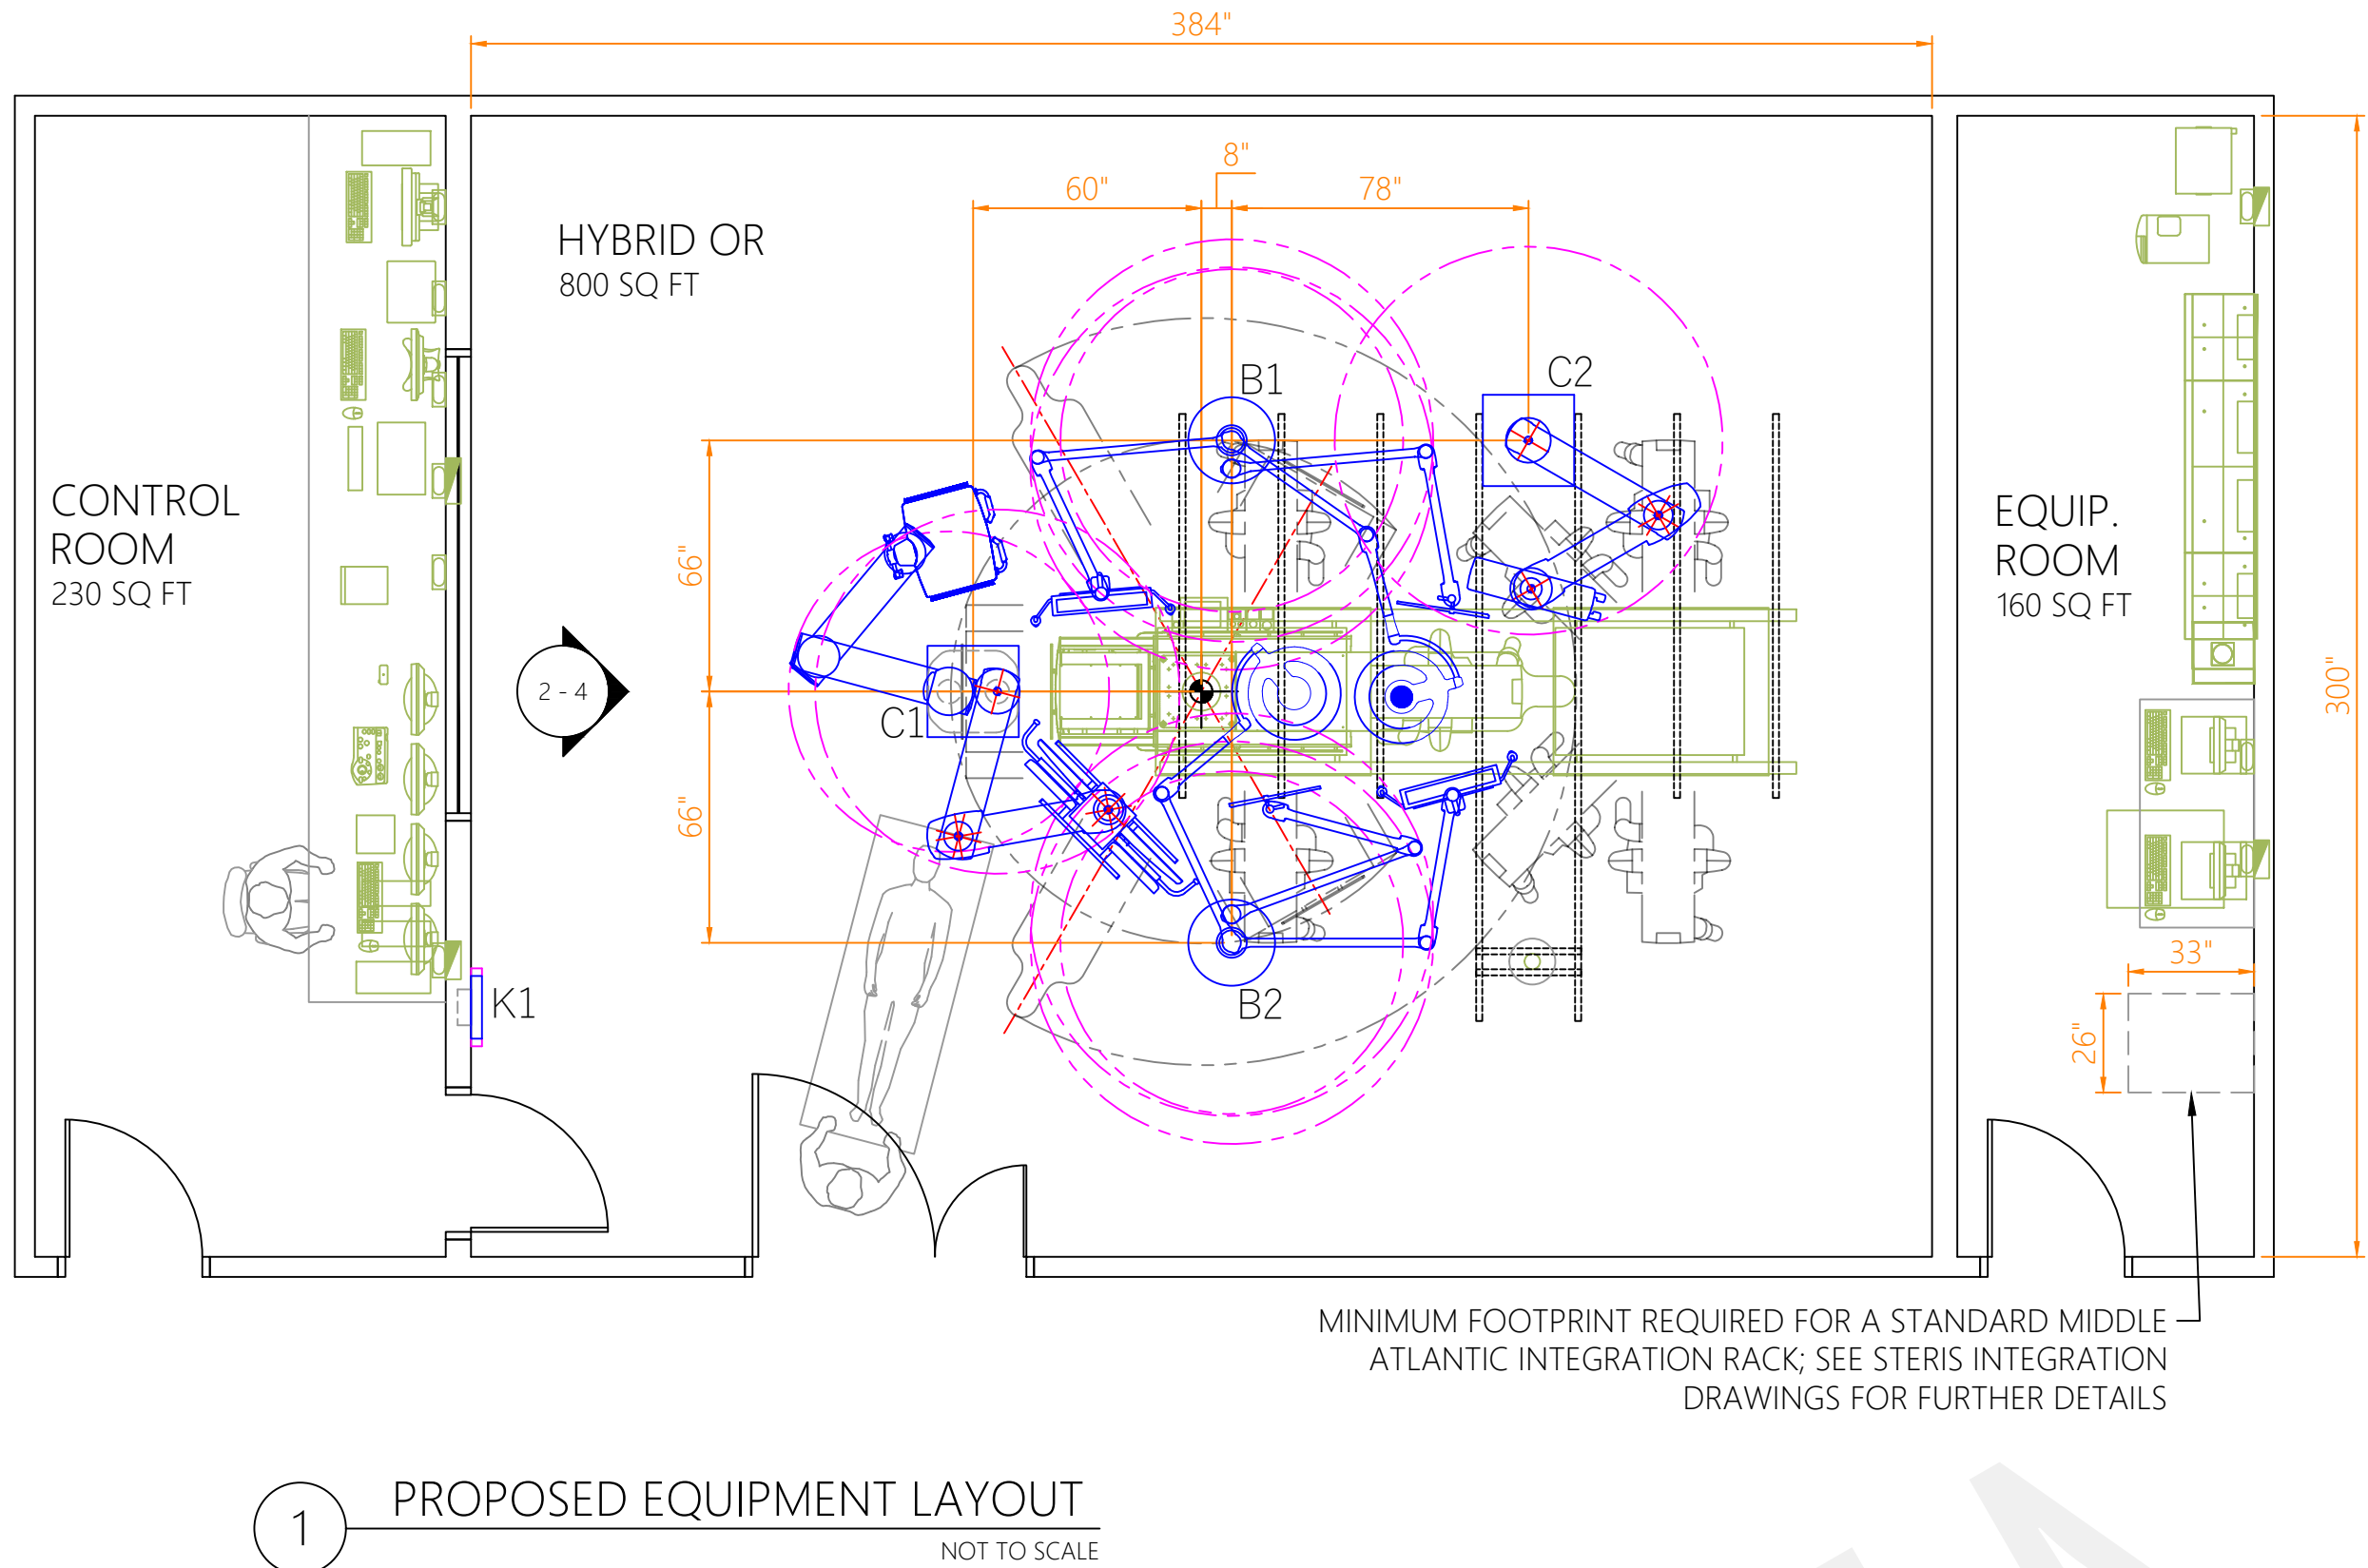


1 PROPOSED EQUIPMENT LAYOUT
NOT TO SCALE

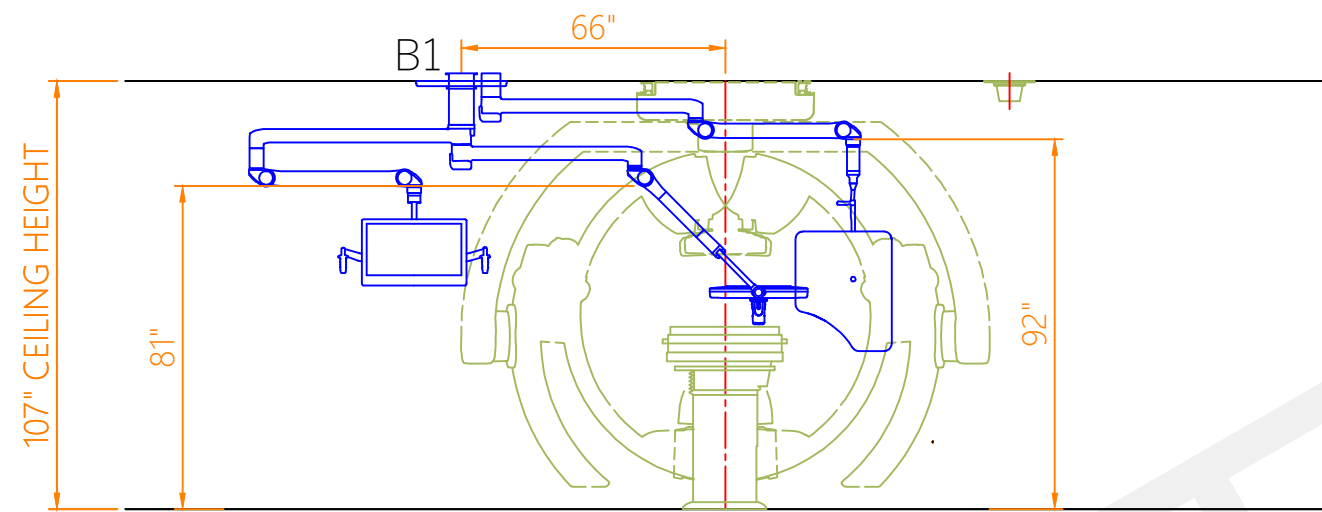

2 FOOT END EQUIPMENT ELEVATION
NOT TO SCALE

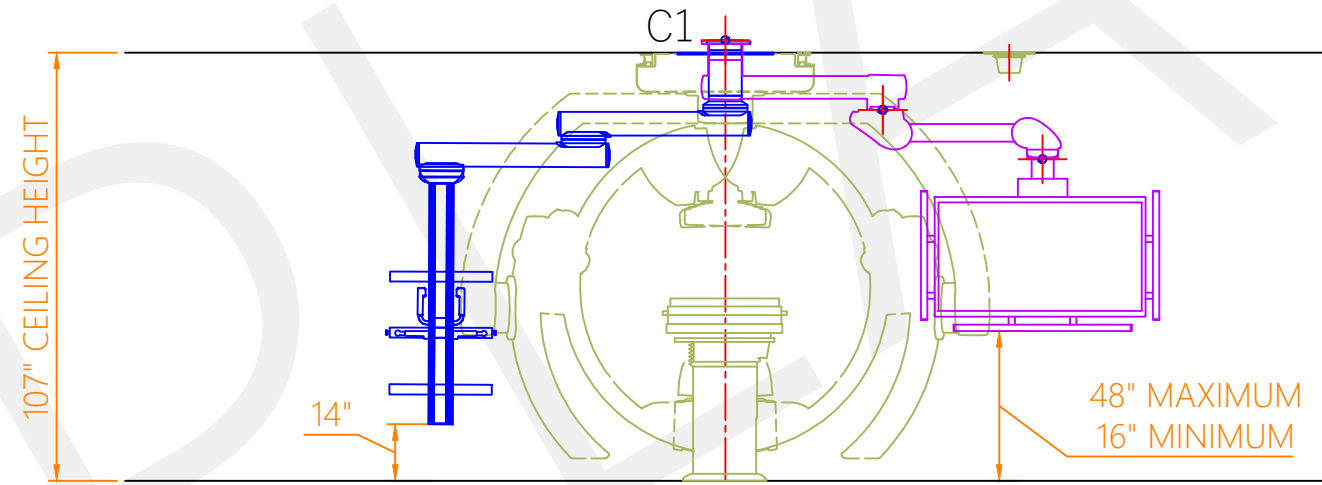

4 FOOT END EQUIPMENT ELEVATION
NOT TO SCALE

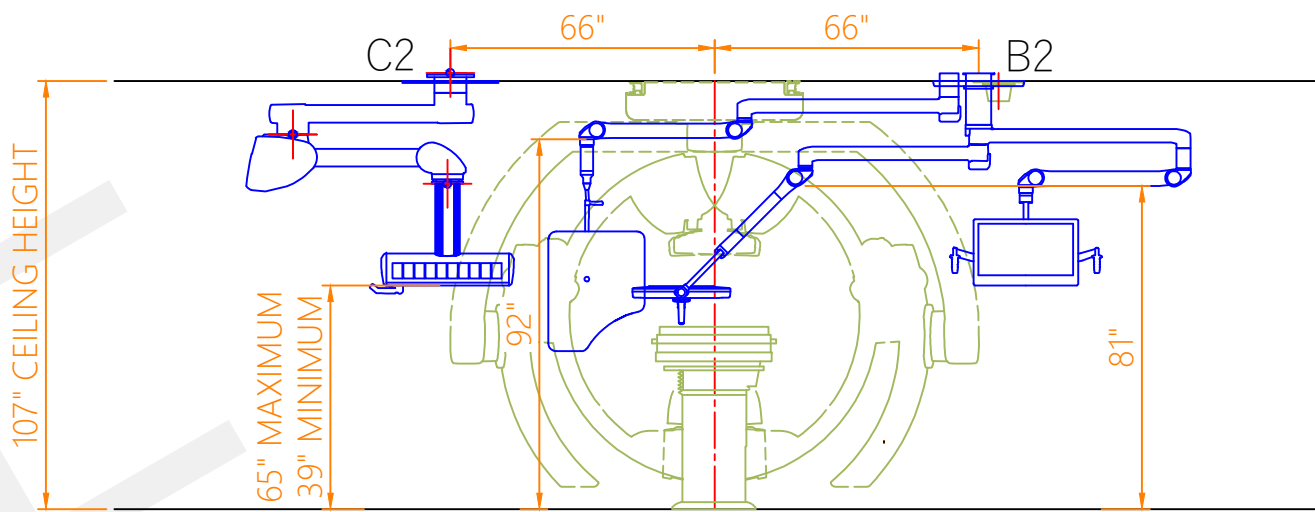

3 FOOT END EQUIPMENT ELEVATION
NOT TO SCALE

EQUIPMENT LIST		
TAG	QTY	DESCRIPTION
B1	1	A Series-Accessory Arm(s), Surgical Light(s) & Accessory Arm(s)
B2	1	A Series-Accessory Arm(s), Surgical Light(s) & Accessory Arm(s)
C1	1	Tandem HarmonyAIR Adj Arm Monitor Carrier - HarmonyAIR Fixed-Equipment, Monitor Carrier
C2	1	HarmonyAIR Adj Arm, Motor Supply Head-Anesthesia
K1	1	HarmonyAIR A-Series Integrated Wall Control

A SERIES LIGHT CONDUIT SCHEDULE			
FROM - TO	QUANTITY	SIZE	RESPONSIBILITY
K1 - B1	2	.75"	ELECTRICAL CONTRACTOR
K1 - B2	1	.75"	ELECTRICAL CONTRACTOR
B1 - B2	CONNECTED VIA FLEX CONDUIT INCLUDED IN SPLIT MOUNT KIT		

LIGHT CONDUIT SCHEDULE NOTES
1. 3/4" CONDUIT FOR AC POWER TO K1.3 CONB. 10AWG WIRE INPUT AC SUPPLY
~120V-240VAC, 7A-3A, 50/60Hz
2. LIGHTING CONDUIT RUNS NOT TO EXCEED 25 FEET
3. CONDUIT REQUIREMENTS FOR LIGHTS ALSO REFERENCED WITHIN THE
EQUIPMENT DRAWINGS FOR THE SPECIFIED SURGICAL LIGHT WALL
CONTROL SYSTEM
4. DC SUPPLY LIGHTHEAD CABLES REQUIRE 1" CONDUIT WHEN DOUBLE RUNS
ARE REQUIRED (LONG RUNS)
5. REFER TO APPROPRIATE EQUIPMENT SPECIFICATIONS TO ENSURE THAT THE
MOST CURRENT & DETAILED INFORMATION OF THIS LIGHT SYSTEM IS
UTILIZED

THIS LAYOUT IS INTENDED TO ENCOURAGE DISCUSSIONS FOR AN INTEGRATED DESIGN PROCESS.
FOR AN OPTIMIZED OPERATING ROOM DESIGN SOLUTION, PLEASE CONTACT YOUR LOCAL STERIS REPRESENTATIVE.
REFER TO THE IMAGING VENDOR FOR ALL IMAGING SYSTEM DIMENSIONS, LOCATIONS, AND REQUIREMENTS.

STERIS drawings do not supersede the drawings from the architect of record.